



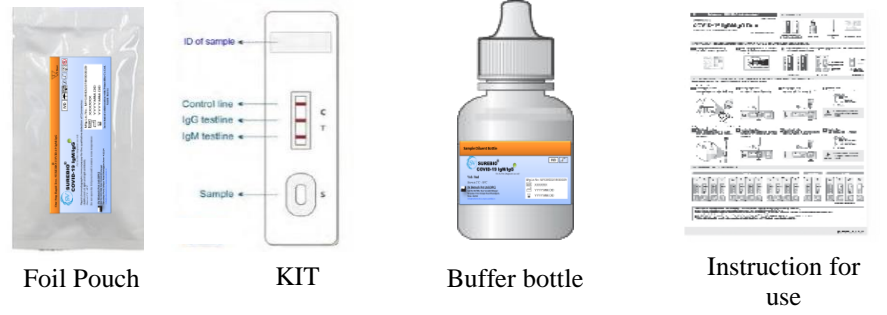


PLEASE READ CAREFULLY BEFORE YOU PERFORM THE TEST

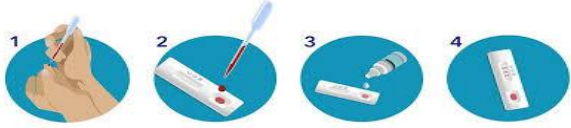


PREPARATION

- Carefully read instruction for using SUREBIO COVID-19 IgM/IgG test
- Open SUREBIO COVID19 IgM/IgG Pouch, and check the test devices and the desiccant in each Pouch



Foil Pouch

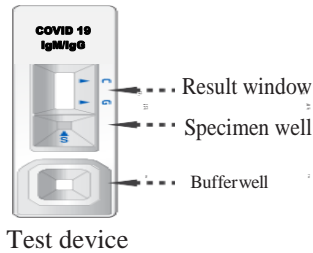

Test device






Desiccant

- Yellow
- Green
- Yellow: Valid
- Green: Invalid

TEST PROCEDURE

- Collecting of Specimen**
Using capillary tube, collect the 10 µl of capillary whole blood to the black line of the capillary tube.
- Adding of Specimen**
Add the collected capillary whole blood to the specimen well of the test device.
- Dropping of Buffer**
Add 3 drops (90µl) of buffer vertically into the buffer well of the test device.
- Reading Time**
Read test result at 10~15 minutes.

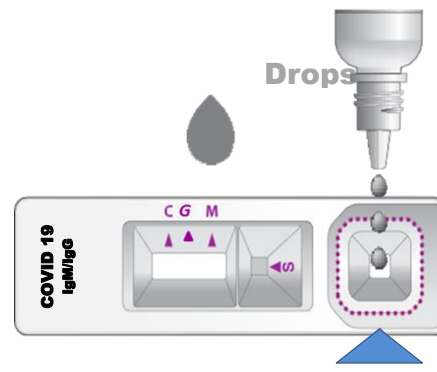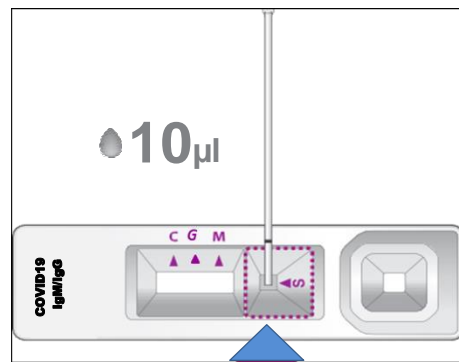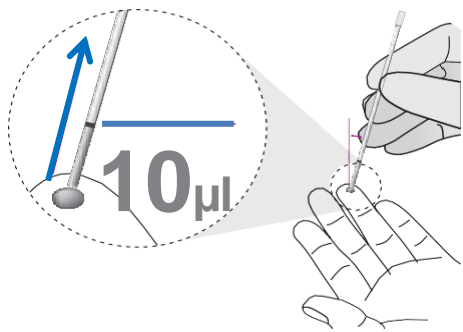

CAUTION Do not read results after 15 minutes. It may give false results

TEST PROCEDURE


- This test should be carried out at the room temperature, hence the test reagent which is stored in the cold storage, should be removed and kept outside 15~30 minutes before the test, so that it is at room temperature.
- Remove the test device from sealed pouch immediately before use.
- Put the test device on a clean table, horizontally placed.
- Using sample transfer pipette/capillary tube, deliver sample 10µL into the sample port on the test device. Then add 3 drops of sample diluent immediately.
- Interpret the result between 10~15 minutes.

STORAGE AND SHELF LIFE
SUREBIO COVID-19 IgM/IgG should be stored at 2~30°C (36~86°F). The test device is sensitive to humidity as well as to heat. Do not use it beyond the expiry date, 24 months from manufacturing date.

INTERPRETATION OF TEST RESULT


Negative

The presence of only 'C' band indicates a negative result

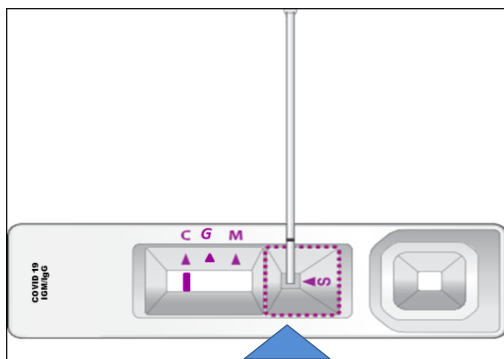


Positive

The Presence of Test band ('M' and/or 'G') with control ('C') band indicates a positive result.

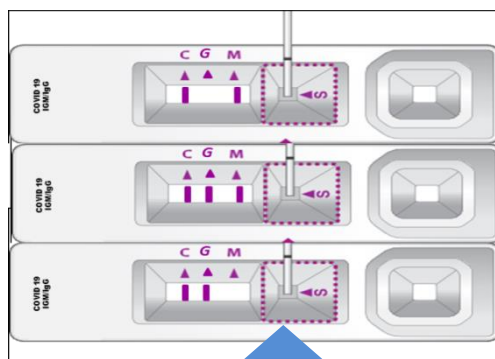

Invalid

If Control (C) band is not appeared in the result window after performing test, the result is considered invalid.

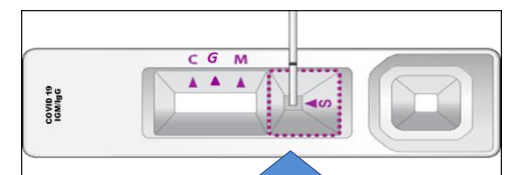

*Re-test with a new test device.

FOLLOW-UP ACTION
As with all diagnostic tests, a definitive clinical diagnosis should not be based on the results of a single test, but should only be made by the physician after all clinical and laboratory findings have been evaluated.

SUREBIO COVID-19 IgM/IgG Test

- A colored band will appear in the top section of the result window to show that the test is working properly. This band is control line (C).
 - A colored band will appear in the lower section of the result window. These bands are test line of IgM/IgG (M, G).
 - Even if the control line is faint, or the test line isn't uniform, the test should be considered to be performed properly and the test result should be interpreted as a positive result.
- * SUREBIO COVID-19 IgM/IgG Test may cross-react with antibody against SARS-CoV-1.
 - * Results from antibody testing should not be used as the sole basis to diagnose or exclude SARS-CoV-2 infection or to inform infection status.
 - * Positive results should be considered in conjunction with the clinical history, RT-PCR results and other data available.

SV Biotech Pvt Ltd (OPC)
Gat No 407/408, Near Sonakshi Mangal
Karyalaya Solapur Road Bhandgaon,
Pune- 412214, 020-26911273/74
info@svbiotech.in, www.surebio.in

In technical collaboration with Prime4Dia Co. Ltd.
South Korea PRIME DIA

